


Sample: Heat Capacity PET Scan
Size: 30.6100 mg
Method: Heat Capacity Scan
Comment: He Purge=25mL/min

DSC

File: C:\TA\Data\DSC\Cpsample.000
Operator: Applications Laboratory
Run Date: 17-Jan-1997 11:01
Instrument: 2920 MDSC V2.2A

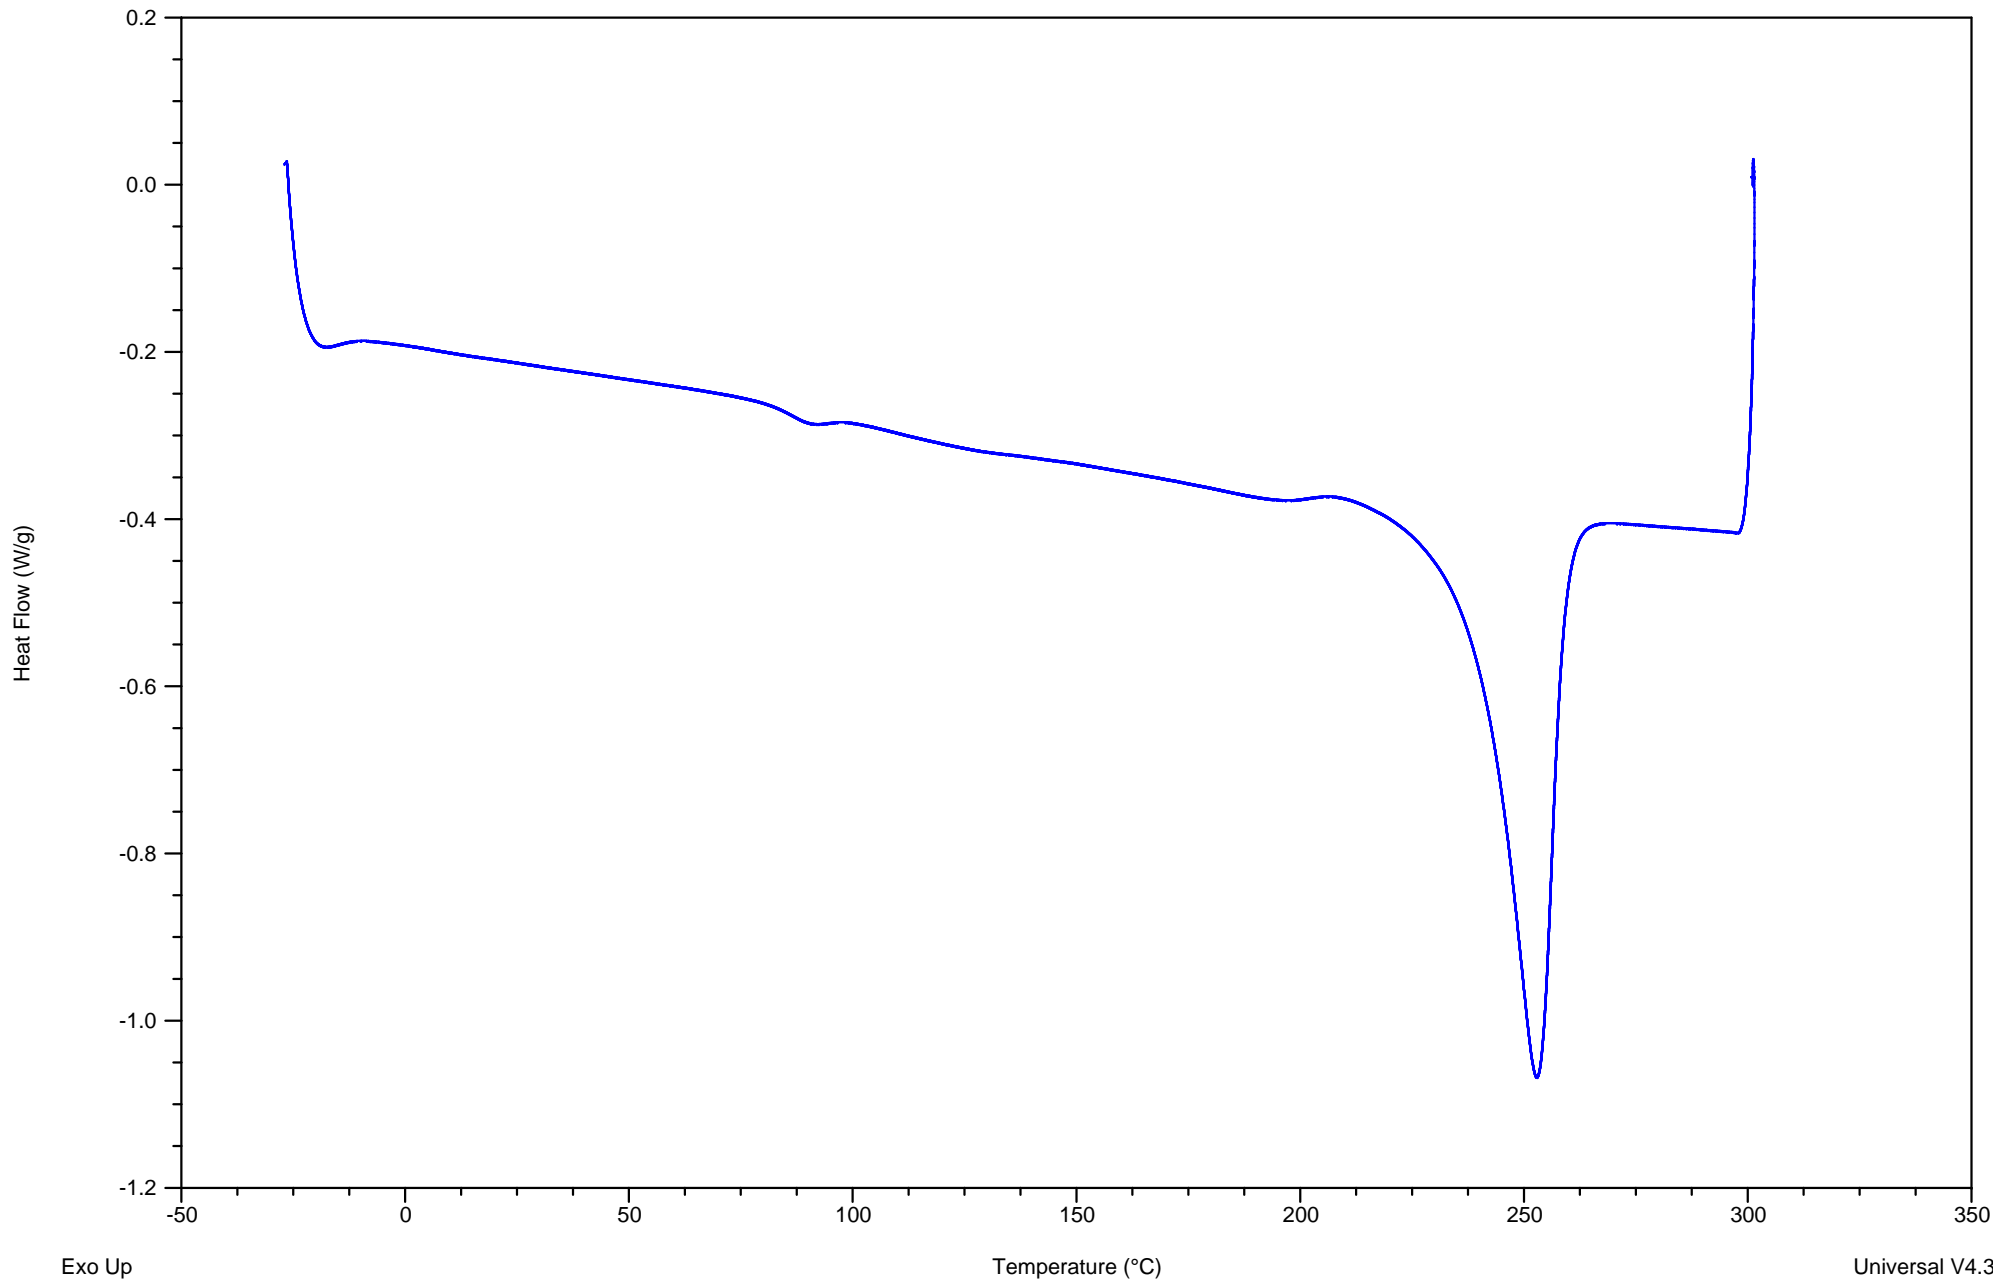

Exo Up

Universal V4.3A TA Instruments